

FIG. 1

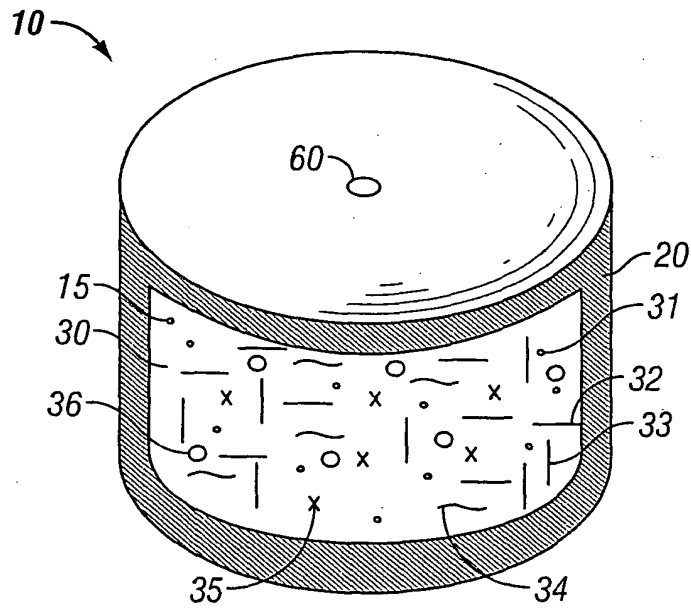


FIG. 2

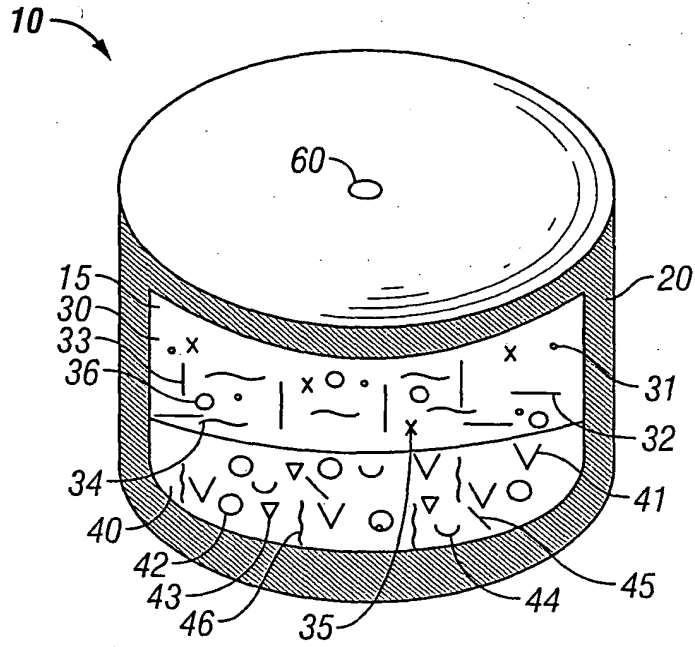


FIG. 3

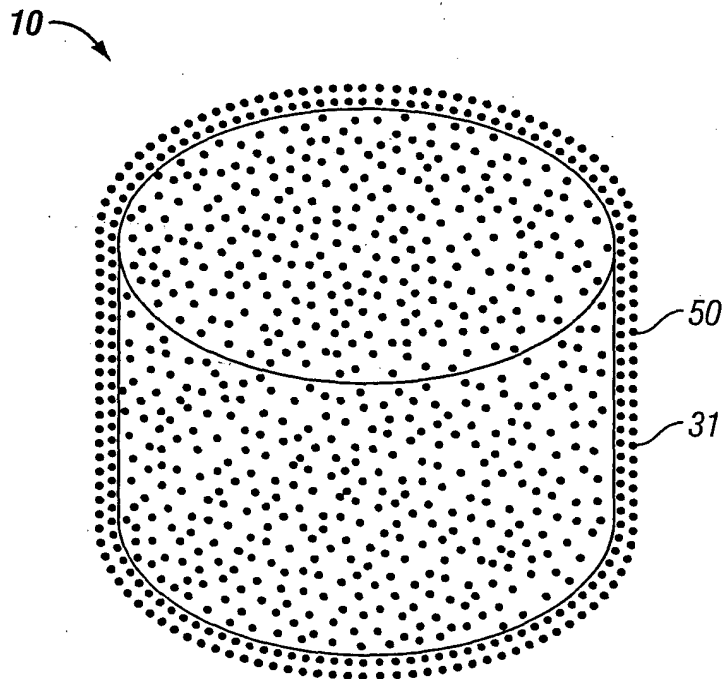


FIG. 4

3/8

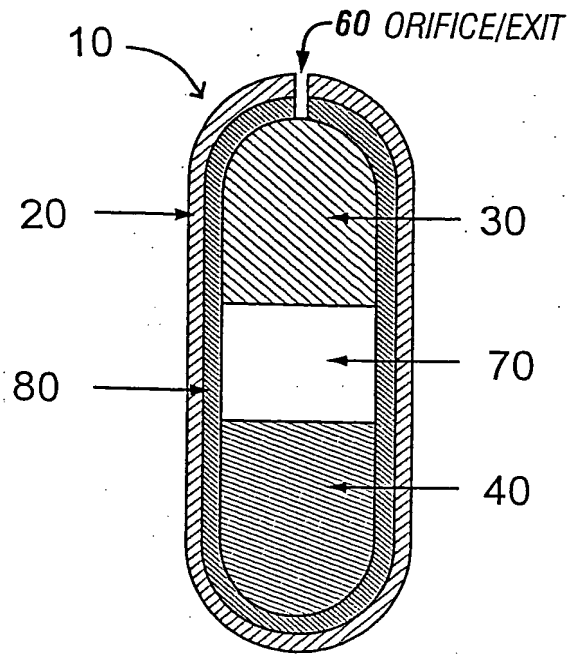


FIG. 5

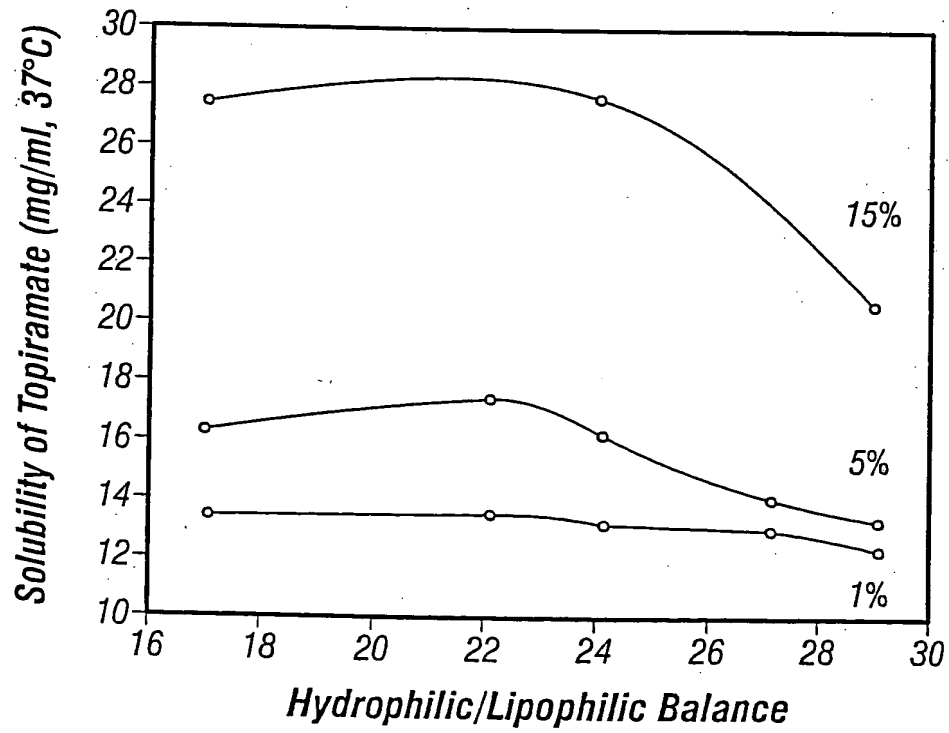


FIG. 6

4/8

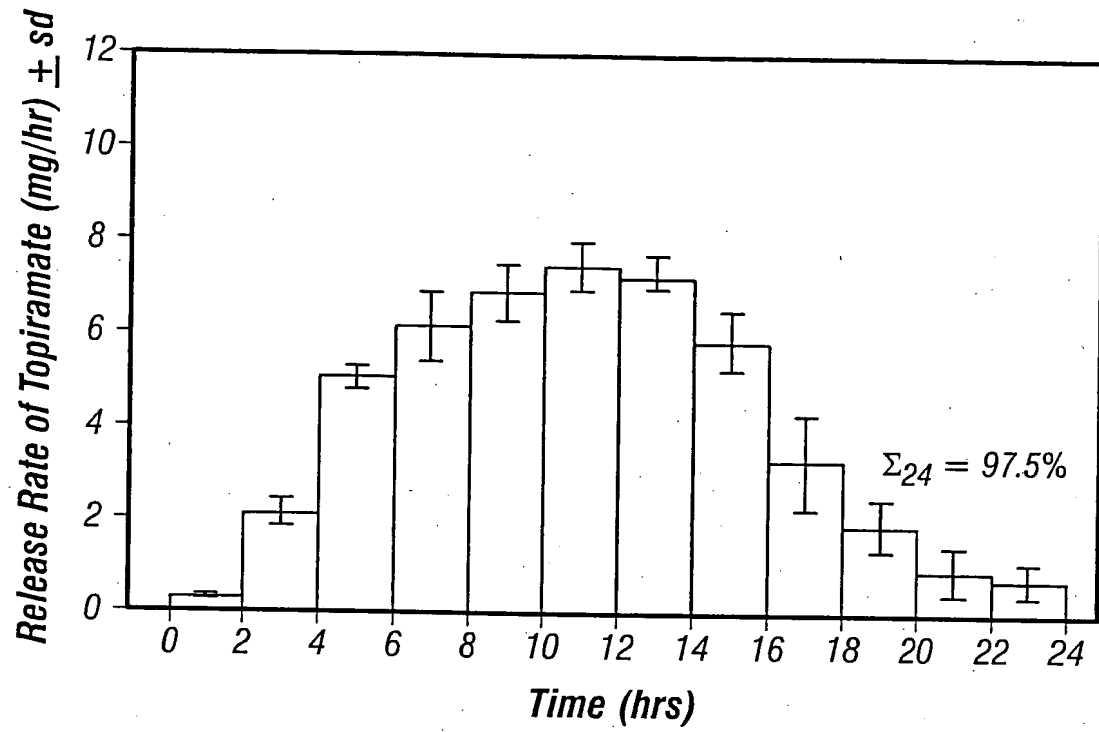


FIG. 7

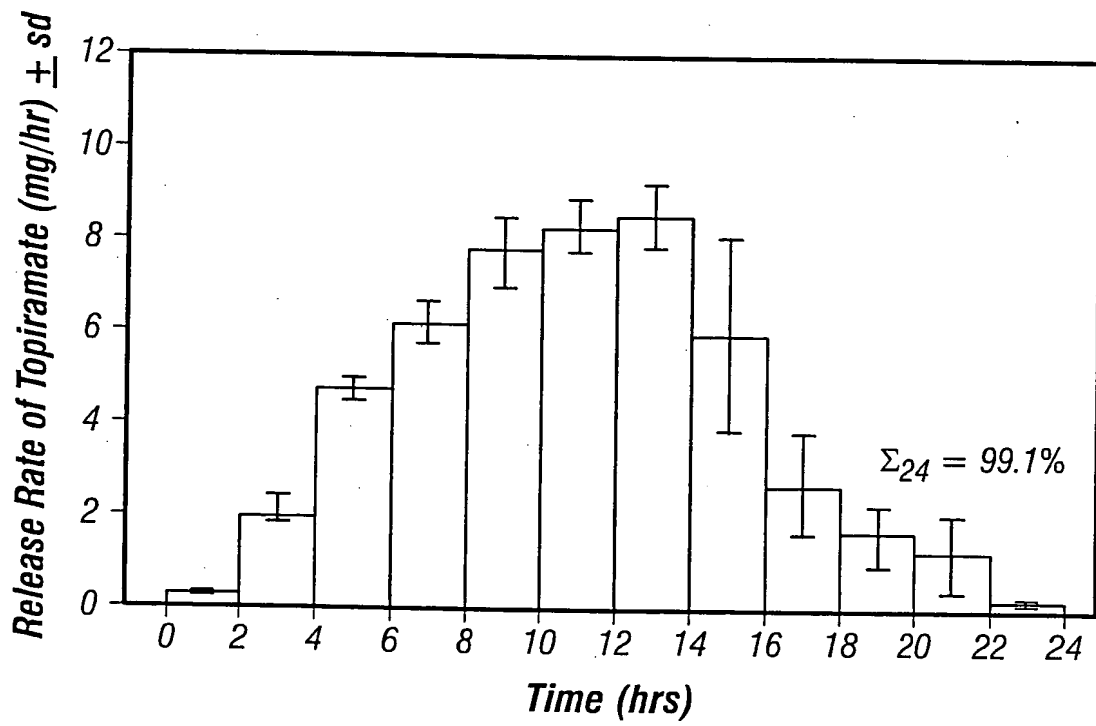


FIG. 8

5/8

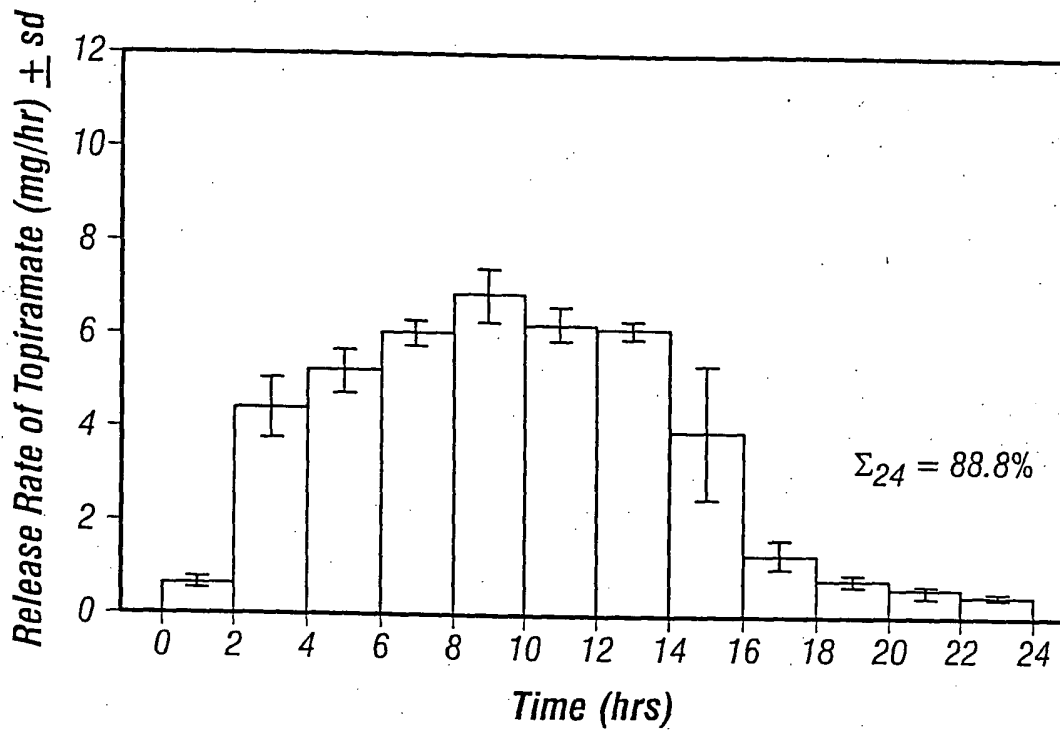


FIG. 9

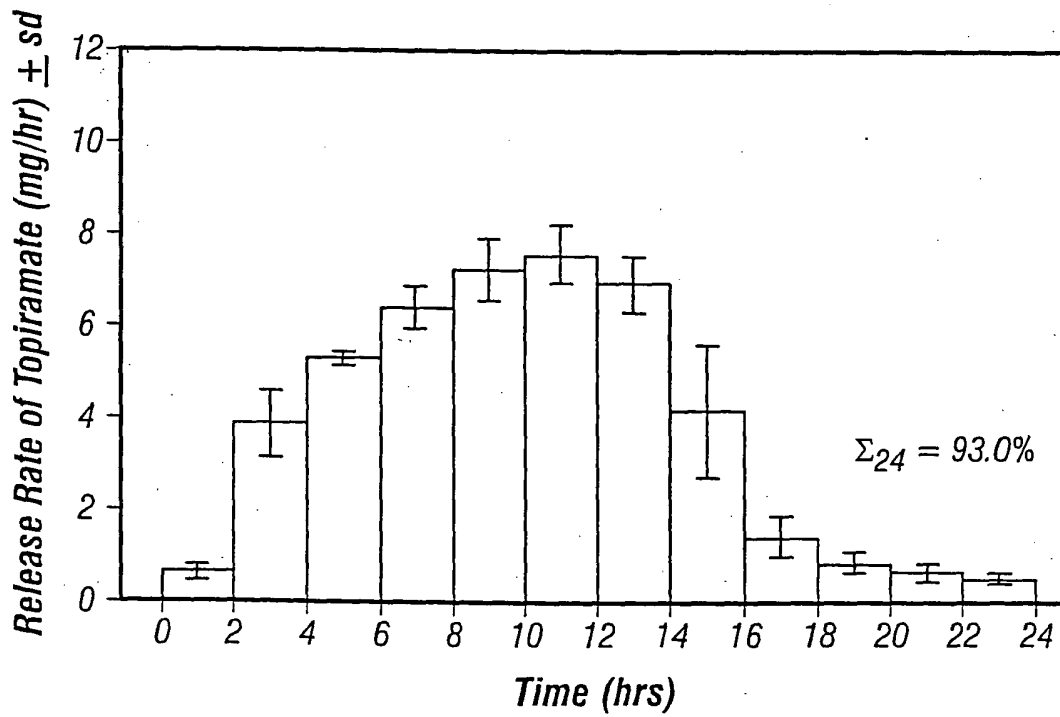


FIG. 10

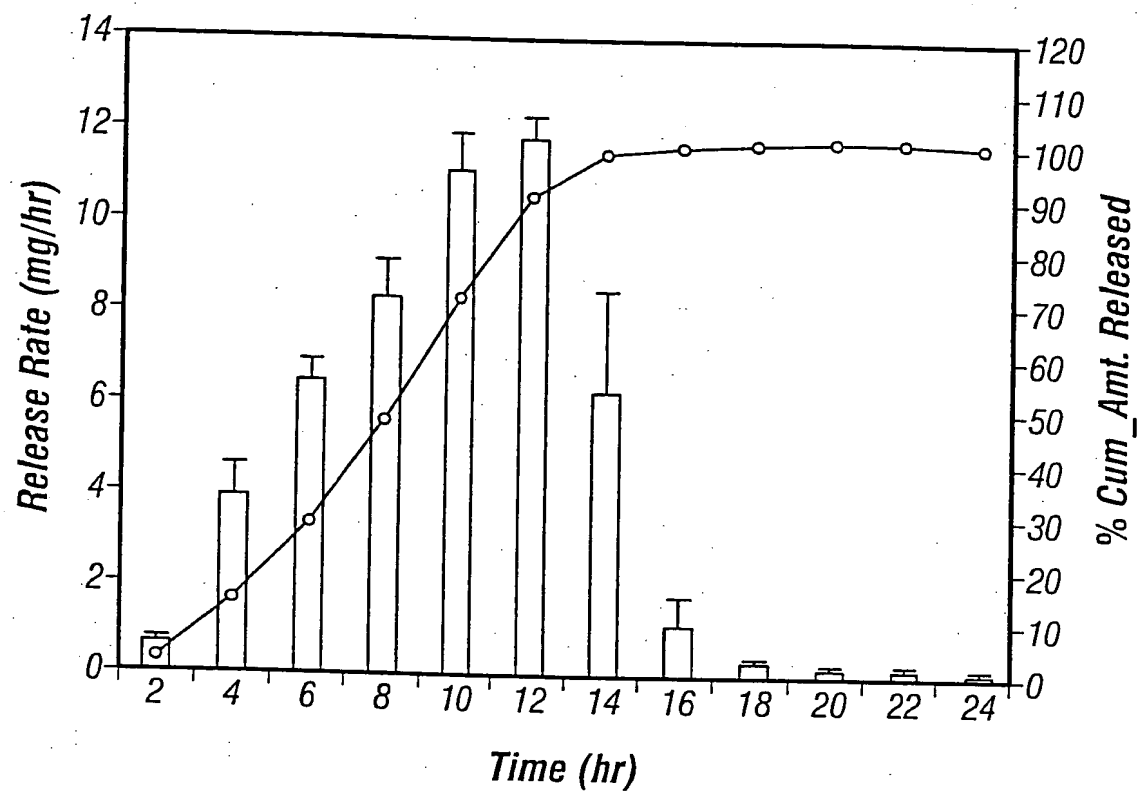


FIG.11

7/8

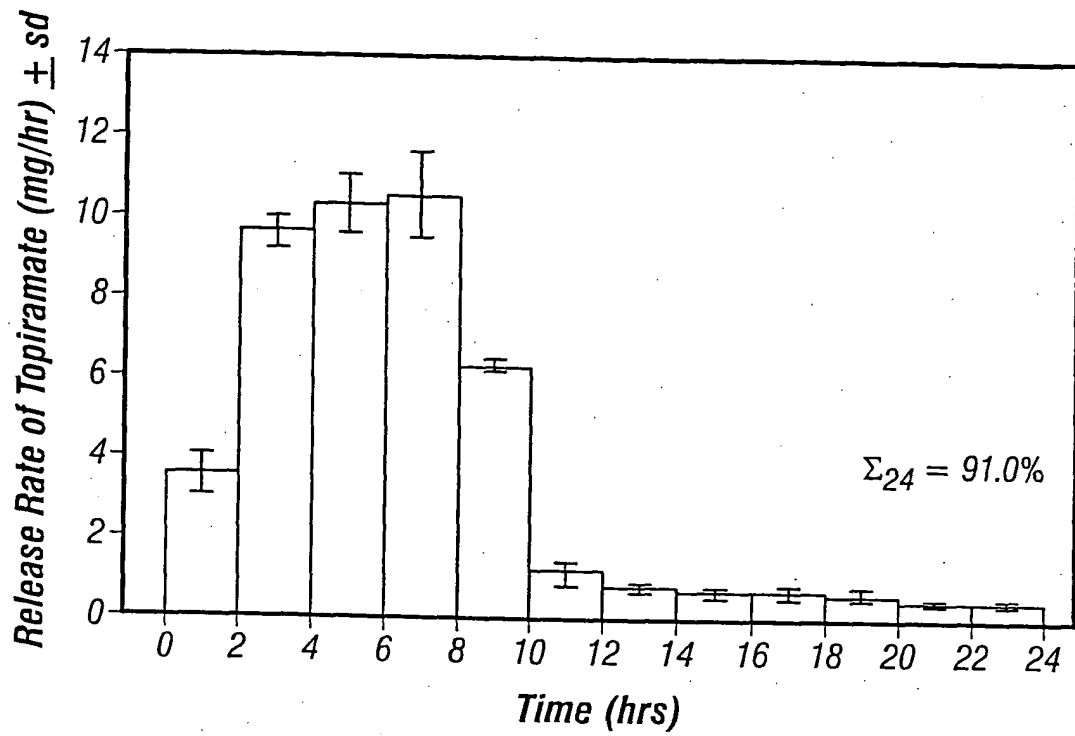


FIG. 12

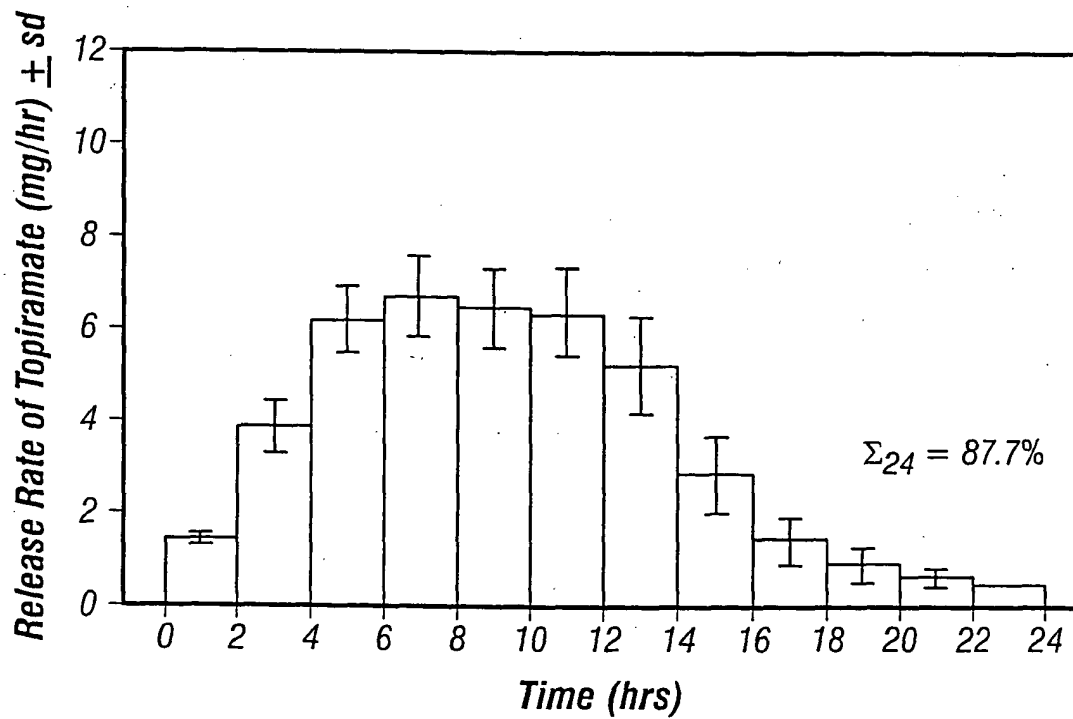


FIG. 13

*Phenytoin*

*Release Rate for Phenytoin Push-Pull System with Drug/Push Ratio of 2.5/1  
D.L. #34 Slow System with Natrosol Subcoat "9"*

*RELEASE MEDIUM: AIF  
NUMBER OF SYSTEMS TESTED: 5  
ORIFICE DIAMETER: 1 x 40 MILS  
DRUG DOSE: 276.00 MG*

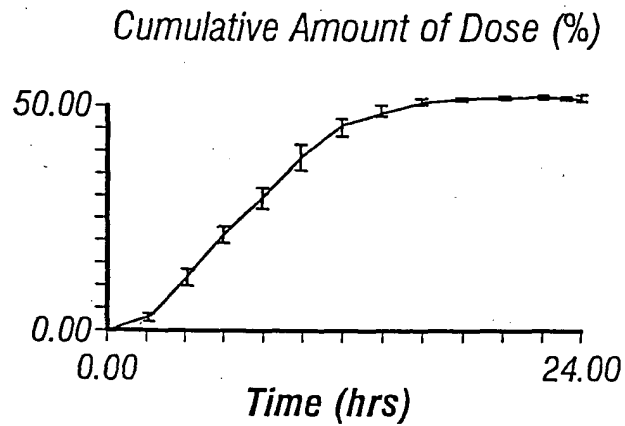
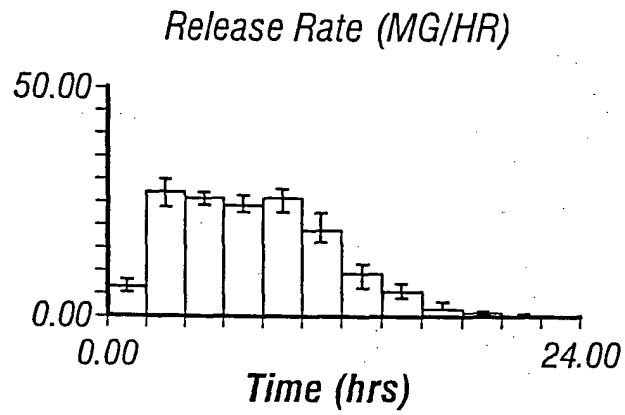


FIG. 14